

Physician: Sample

Patient: Sample

Accession #:

Age: 56


Sex: F

Assay Batch #: Sample Report

Collected: 04/29/09

Received: 05/04/09

Completed: 05/07/09

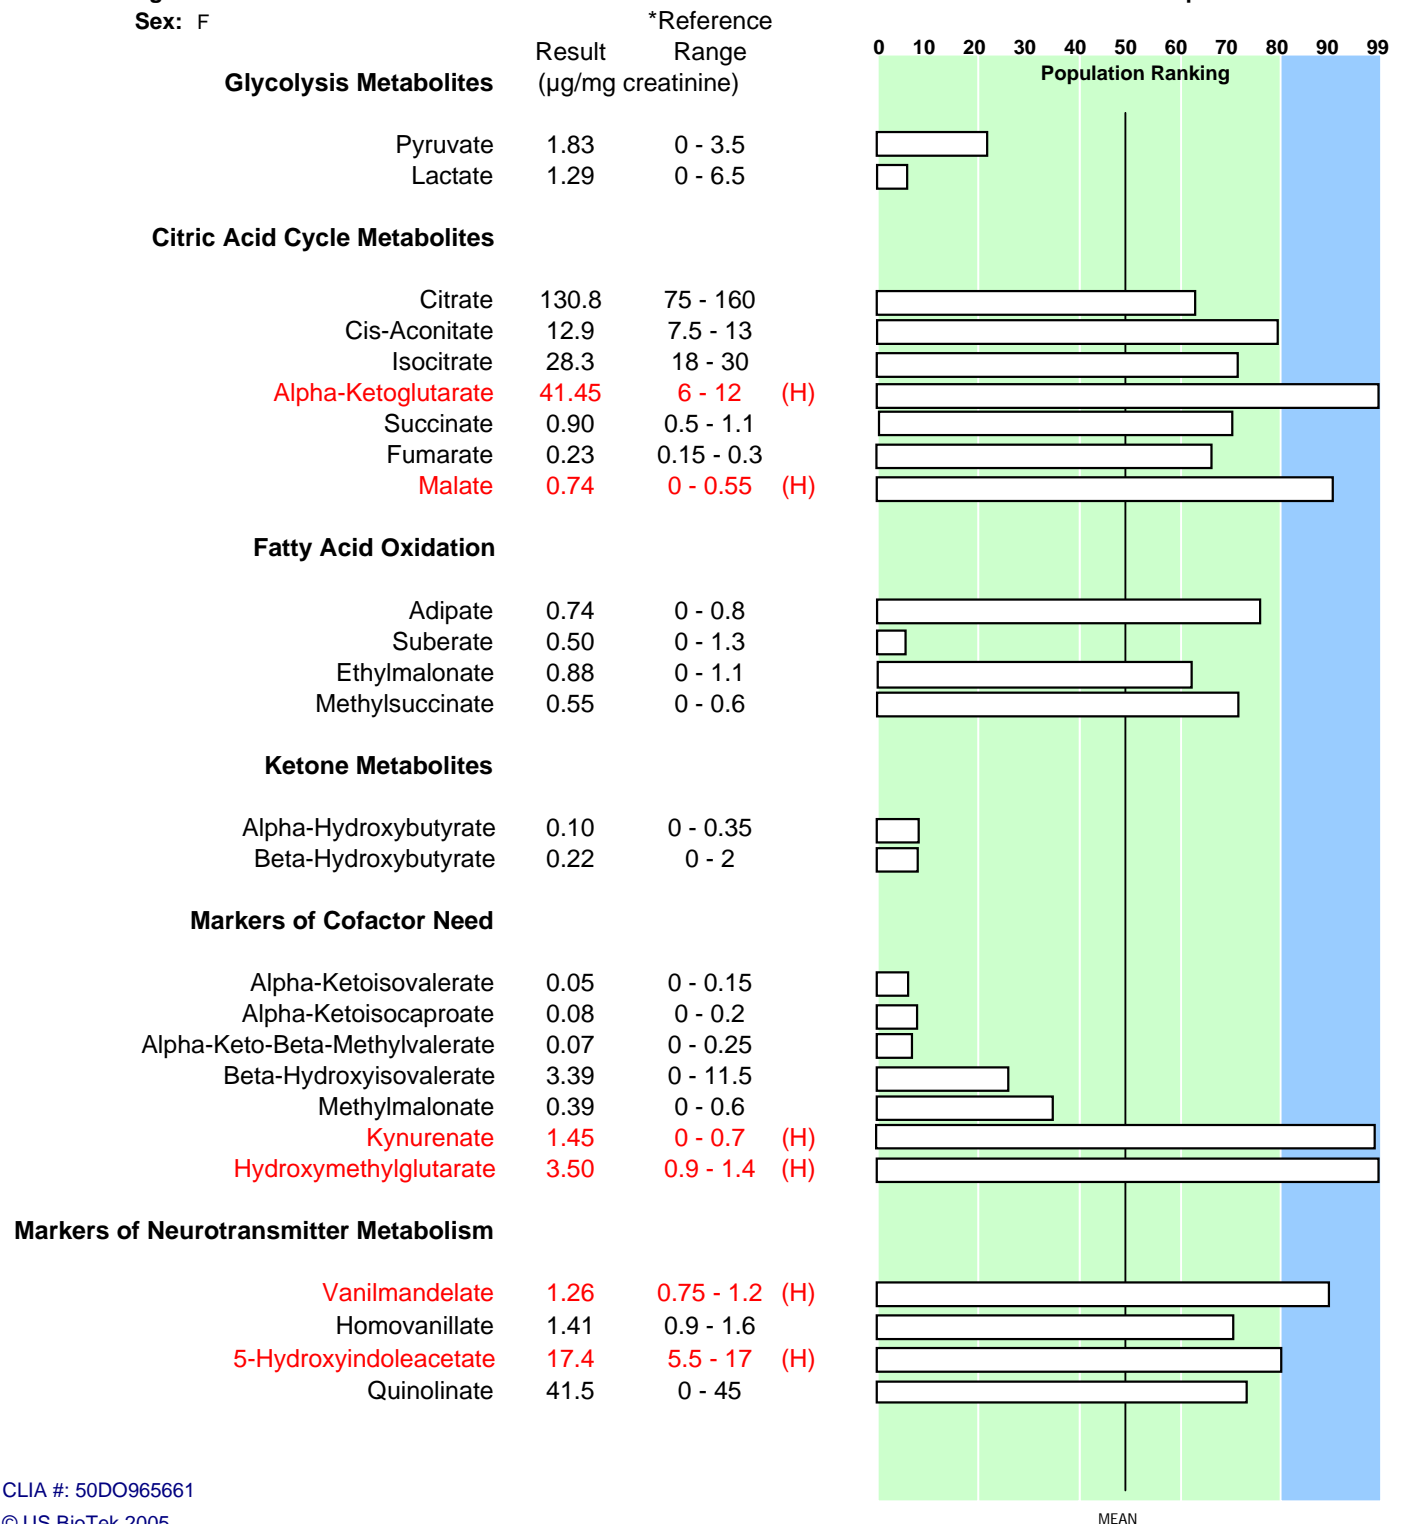

CLIA #: 50DO965661

© US BioTek 2005

ND is none detected


*Reference ranges are gender specific and results are age adjusted for children

US BioTek Laboratories has developed and determined the performance characteristics of this test. This test is not intended to diagnose, treat, or prevent any disease or replace the medical advice and/or treatment obtained from a qualified healthcare practitioner. This test has not been evaluated by the U.S. Food and Drug Administration. This test does not assess for neonatal inborn errors of metabolism and is based on stable renal function and normal renal clearance.

Physician: Sample
Patient: Sample
Accession #:
Age: 56
Sex: F

Assay Batch #: 090506oaG
Collected: 04/29/09
Received: 05/04/09
Completed: 05/07/09

Reference range updated 1/26/2009

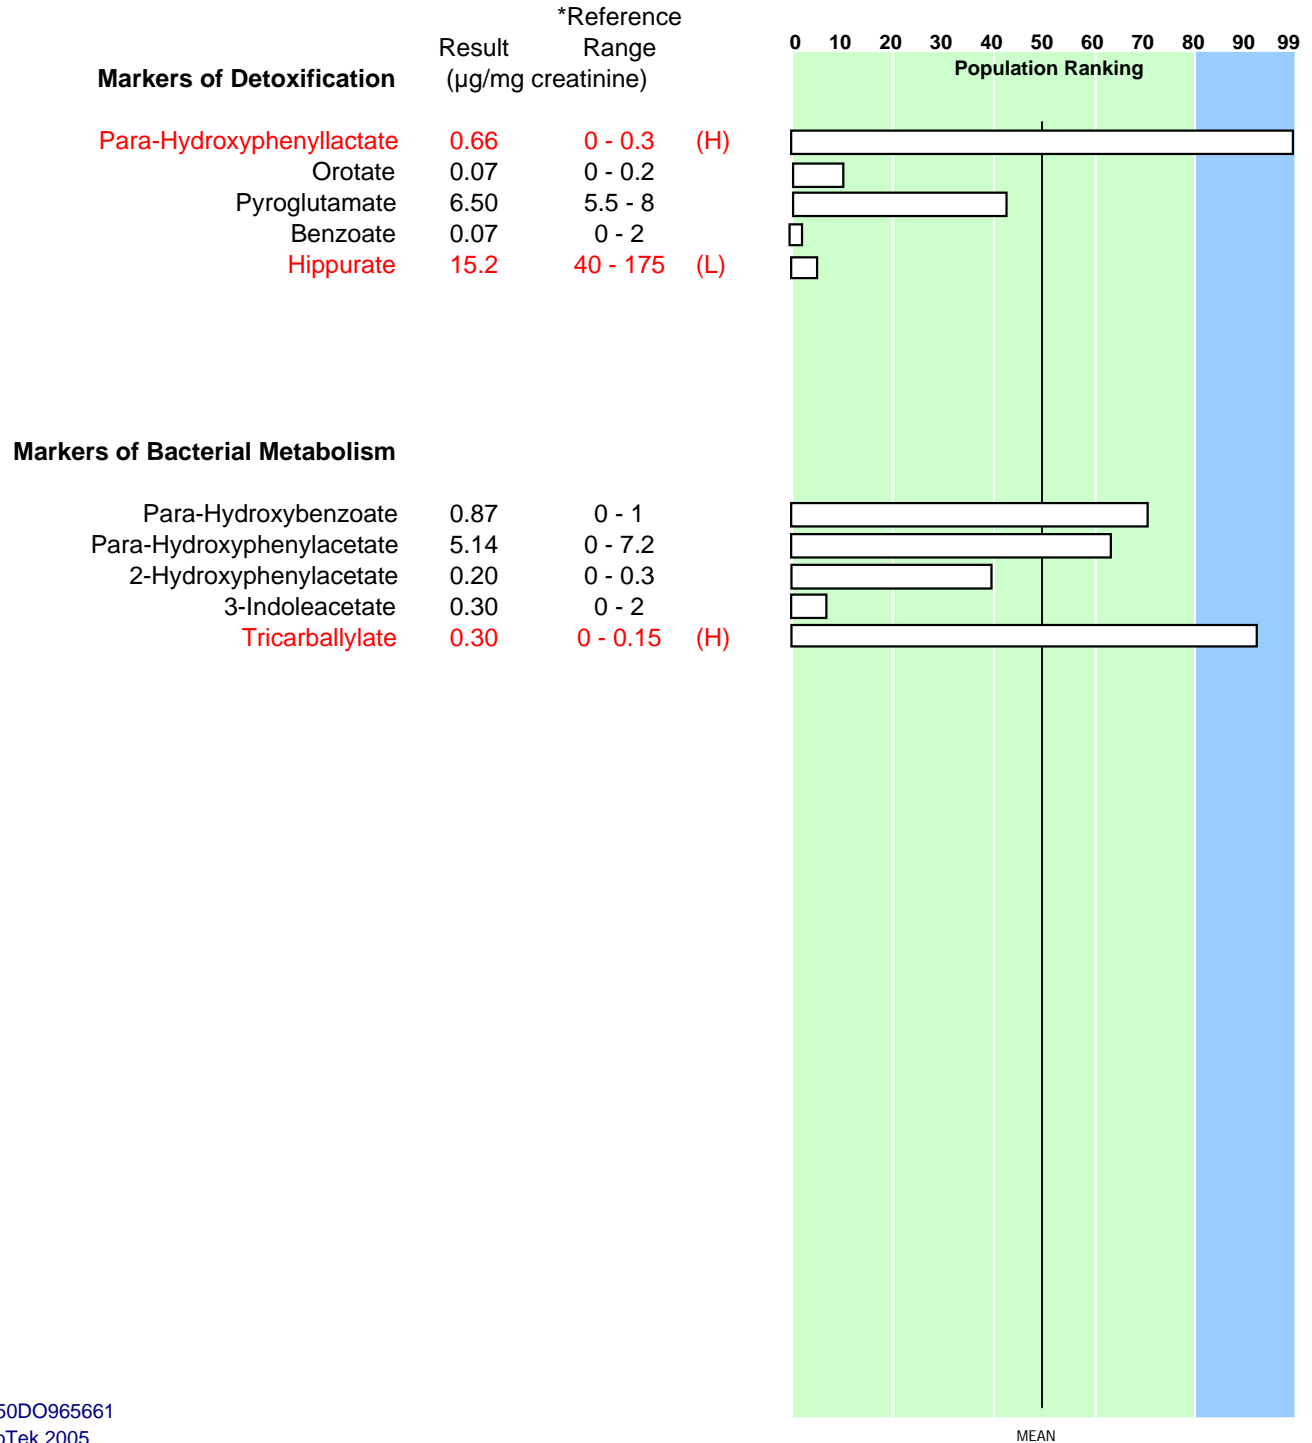

CLIA #: 50DO965661

© US BioTek 2005

ND is none detected

The analytes on the panel are subject to change without prior notice

*Reference ranges are gender specific and results are age adjusted for children

US BioTek Laboratories has developed and determined the performance characteristics of this test. This test is not intended to diagnose, treat, or prevent any disease or replace the medical advice and/or treatment obtained from a qualified healthcare practitioner. This test has not been evaluated by the U.S. Food and Drug Administration. This test does not assess for neonatal inborn errors of metabolism and is based on stable renal function and normal renal clearance.