US BioTek LABORATORIES

16020 Linden Ave North, Shoreline, WA 98133, USA

15 Mold Panel + Total IgE*: IgE

Complete Report

Provider: Sample Report
Patient:
Accession #:
Collected:

Sex:
Age:
Received:

Sample Type: Serum
Date of Birth:
Completed:

IgE [redacted]

CLIA #: 50D0965661
COLA accredited

Molds

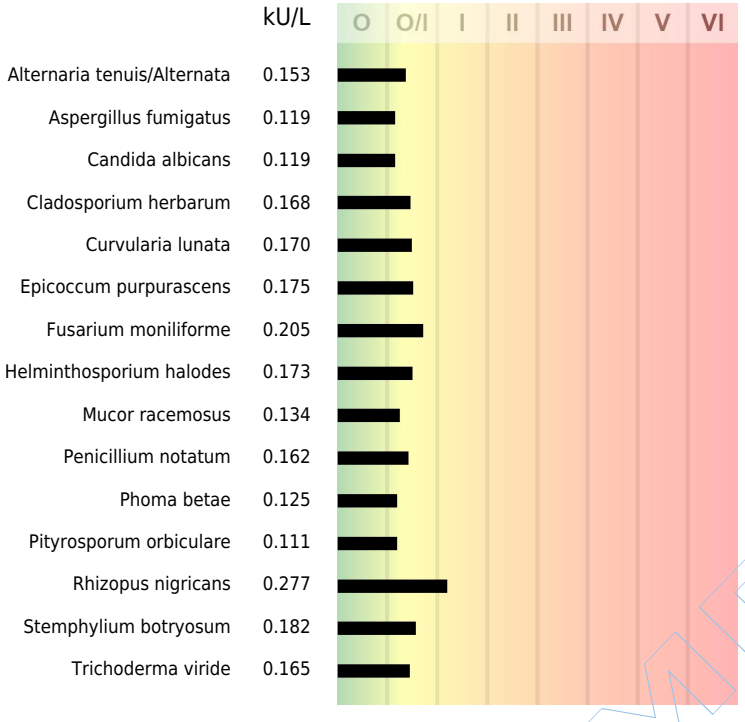

Total IgE*: 19.2 IU/mL

Reference Range:

≥10 years: ≤87.0 IU/mL

<10 years: Not available

Reaction Class

Director: Jillian Harrington, PhD, HCLD (ABB)

O	O/I	I	II	III	IV	V	VI
<0.10	0.10-0.24	0.25-0.39	0.40-1.29	1.30-3.89	3.90-14.99	15-24.99	≥25
Absent or Not Detectable	Very Low	Low	Moderate	High	Very High	Very High	Very High

*The Total IgE is performed using Immulite System, and the reference range is updated accordingly. The IgE Chemiluminescent assay used by US BioTek Laboratories has been cleared by the U.S. Food and Drug Administration. The performance characteristics of the IgE assay has been verified by US BioTek Laboratoriess, LLC, 16020 Linden Ave N, Shoreline, WA 98133, USA. IgE test results should be used in conjunction with other relevant clinical information by healthcare providers to diagnose IgE-mediated allergic disorders. Higher total IgE levels may suggest elevated clinical reactivity to specific foods but should be interpreted in conjunction with other relevant information.